




This product is available through:
JRT Associates
 800-221-0111

**UNMATCHED
 SOLUTIONS
 FOR QUALITY
 CONTROL**

Pro-NM DualSource

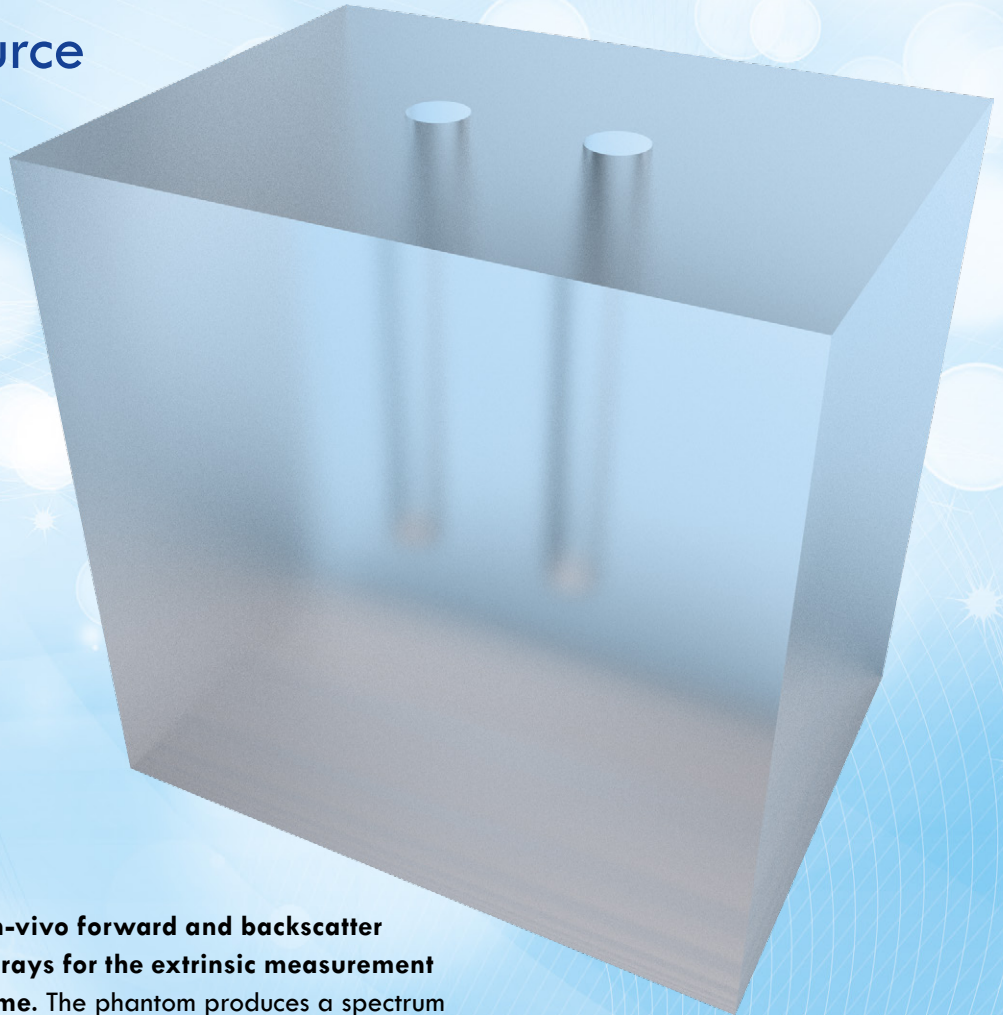

This scatter phantom simulates in-vivo forward and backscatter characteristics of 99 mTc gamma rays for the extrinsic measurement of a scintillation camera's deadtime. The phantom produces a spectrum typical of that observed from 99 mTc in the myocardium.

Reference: Ralph Adams, Gerald J. Hine, and C. Duane Zimmerman, "Deadtime Measurements in Scintillation Cameras Under Scatter Conditions Simulating Quantitative Nuclear Cardiology," *The Journal of Nuclear Medicine*, 19 (1978), 538-544.

**Technical data
 (can be modified to customer specifications):**

- made of PMMA
- dimensions: 150 x 200 x 200 mm
- the two holes are used to hold the radioactive sources
 - hole dimensions: \varnothing 17 mm x 120 mm deep
 - spaced 50 mm apart (center-to-center)
 - distance from the face of the phantom: 50 mm

Product features:

- Complies with:
 - NEMA Standards Publication (NU 1-2001) Performance Measurements of Scintillation Cameras
 - NEMA Standards Publication (NU-1 2007) Gamma Cameras
 - AAPM Report No. 9 - Computer Aided Scintillation Camera Acceptance Testing
 - AAPM Report No. 22 - Rotating Scintillation Camera SPECT Acceptance Testing and Quality Control
 - ACR-SNM (Res. 5 – 2011) technical standard for diagnostic procedures using radiopharmaceuticals
- CE certified
- the Manual provides detailed guidelines for carrying out each test, results assessment and registration

